


Alpha DESIGN® BK Liners Order Form Important Casting & Marking Guidelines

This form will allow you to order an Alpha DESIGN® Liner with custom modifications for either a "Standard" shaped BK limb or for a "Symes" shaped BK limb. Below are diagrams that explain what the custom profile of each type will be. For greater control over the design ask WillowWood about the OMEGA® Scanner 3D and the Alpha DESIGN Liner wizard.

Maximum of 25 mm thickness.



For a standard Alpha DESIGN BK Liner from a cast, the standard base gel would be:

- 6 mm base thickness
- 9 mm distal thickness over the distal fibula and tibia
- 3 mm proximally above the socket
- 3 mm posteriorly behind the patella
- 9 mm over the fibula head

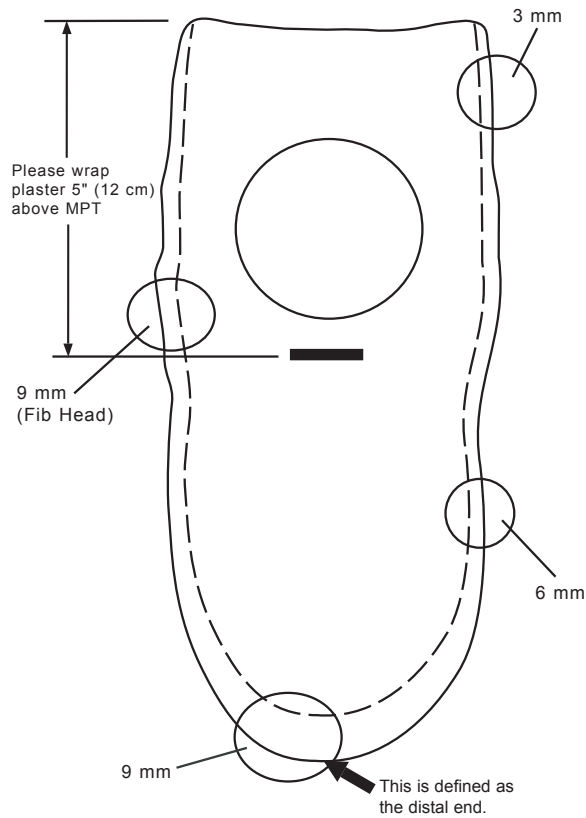

For a Symes Alpha DESIGN BK Liner from a cast, the standard base gel would be:


- 3 mm base thickness
- 3 mm of proximally above the socket
- 3 mm posteriorly behind the patella
- Up to 25 mm to fill the necking area above the malleolus
This area will be filled to create a more cylindrical shaped limb
- 6 mm over fibula head

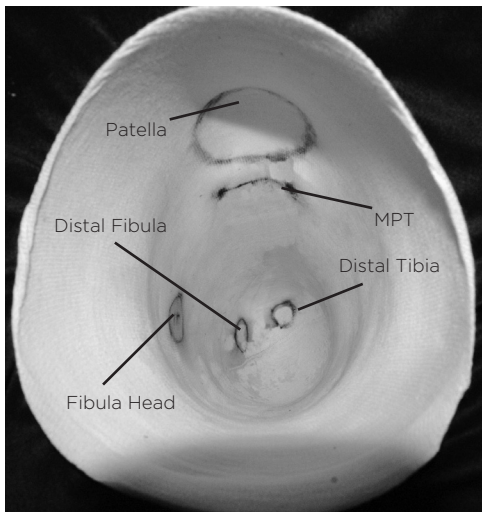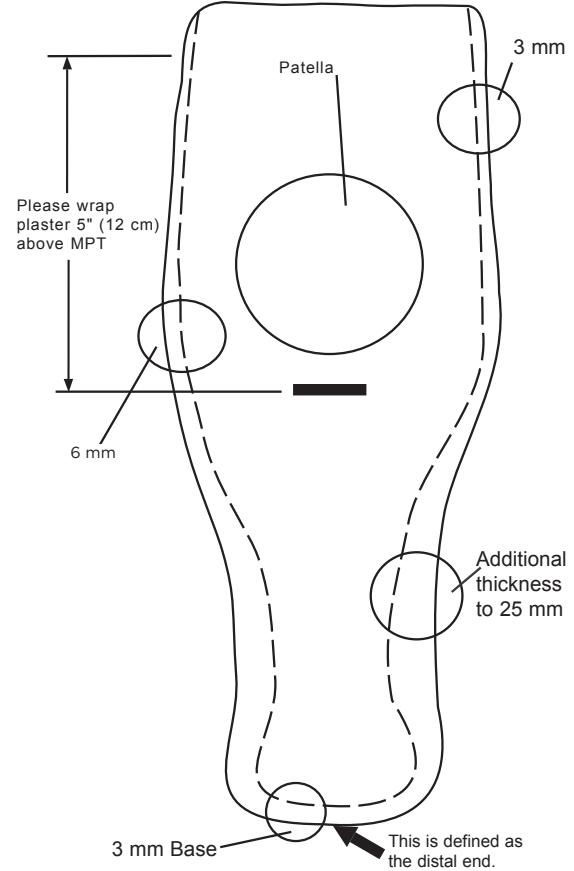

Proximal View

See the examples for the marks that must be indicated on the cast.

Missing marks may result in no additional gel at the location and may delay the order.

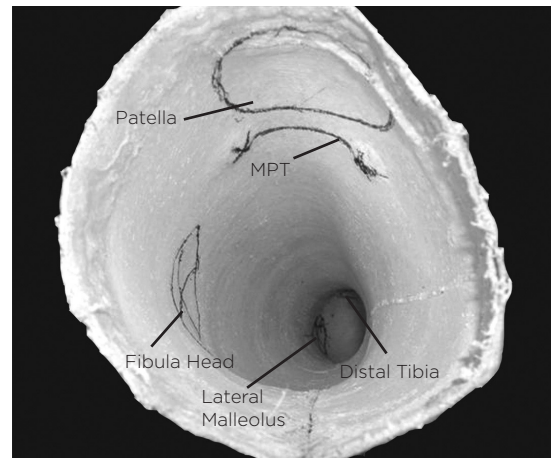

Please Note:

- For bilateral amputees, please use separate forms for each residual limb for best socket/liner accuracy.
- When casting, please cast patient at least 4" to 5" above the knee.
- Please make sure to include the patient ID on the cast.